



Review paper

## Short review on hydroxyapatite powder coating for SS 316L

Jashanpreet Singh<sup>1,✉</sup>, Jatinder Pal Singh<sup>2</sup>, Satish Kumar<sup>3</sup> and Harjot Singh Gill<sup>4</sup>

<sup>1</sup>University Center for Research & Development, Chandigarh University, Mohali 140413, India

<sup>2</sup>School of Mechanical Engineering, Lovely Professional University, Phagwara 144411, India

<sup>3</sup>Department of Mechanical Engineering, National Institute of Technology, Jamshedpur 831014, India

<sup>4</sup>Department of Mechanical Engineering, Chandigarh University, Mohali 140413, India

Corresponding author: ✉ [ijashanpreet@gmail.com](mailto:ijashanpreet@gmail.com); [jashanpreet.t1764@cumail.in](mailto:jashanpreet.t1764@cumail.in)

Received: November 22, 2022; Accepted: December 10, 2022; Published: January 14, 2023

### Abstract

Medical implants and other biomaterials are used by millions of individuals all over the globe to restore lost bodily functions due to injury or illness. Many of these implants fail after a short time or have difficulties, despite the fact that they play important roles in keeping a person's life safe or increasing the quality of their lives. It is the lack of biocompatibility that has proven to be the biggest downfall of biomaterials. Investments in this industry may be made using a thin film of hydroxyapatite powder (HAP) on stainless steel. Plates, screws, pins, and artificial joints are only some fixation devices for bones that often use 316L stainless steel. However, due to its unique advantageous qualities such as super-elasticity and low-profile feature, thin film HAP signals a high potential for use in compact new cardiac devices like the cardiovascular system and protecting stent grafts.

### Keywords

Biomaterials; biocompatibility; implants; plasma spray; coatings

### Introduction

The bones, joints, and teeth that make up the human skeletal system may heal from a broad range of ailments with basic care. There has been a dramatic increase in the complexity of orthopedic injuries since the advent of industrialization. Orthopedic surgery may be necessary to repair or replace a broken bone. Above 500,000 joints are replaced each year in the USA alone, and thousands of patients have this procedure every year globally [1]. The average demand for complete implants is anticipated to rise by almost 30 % over the next decade and a half [2]. There will be an increase from 10.1 million to 13.9 million people living with osteoporosis between 2002 and 2020 [3]. As a result, Ti-based alloys, stainless steel, and alumina/zirconia ceramics have been the only biomaterials employed in these implants up to this point [4]. Bone cement, used for affixing joint prostheses, is a common component of such treatments. Bone cement is used to fill bone and dental cavities using self-curing polymers, and they also serve as load distributors for implants. Due to its bio-stability and high mechanical

qualities, poly(methyl methacrylate) is used in this sector since the 1960s [5]. It is essential to mimic the composition and structure of genuine bone to achieve features comparable to those of natural bone. In order to do this, it is necessary to study the anatomy of real bone [6].

Coating is the technique used to improve the mechanical properties of a surface. This method is also used in biomedical applications where metal implants predominate. Despite the fact that metal devices offer beneficial features, including higher strength, corrosion-resistant, and biocompatible properties within the human body, they are nonetheless not without their drawbacks. These gadgets still used metal and were rusted in varying conditions. Because of its great stability and biocompatibility, hydroxyapatite (HAP) is often used as a coating for metal implants [7]. It is well-known that steel corrodes in moist settings like the human body. So, Babu *et al.* [8] use a dip-coating technique to attempt to improve the bioactive coating of implants. SS316L steel was used as a base material with HAP made of biphasic calcium phosphate for the experiments. Before anything else, specimens of the substrate were heated for 15 minutes in a solution containing 20 % of  $\text{HNO}_3$  at 600 °C to create nonreactive substrate surfaces. Substrate specimens were then submerged in the  $\text{HNO}_3$  based solution to start the coating. Results showed that utilizing this approach at the right temperatures will strengthen the adherence of the coating to the base material.


Many scientists have tried utilizing ceramic powders as additives to coating solutions to form a protective layer on metals since thermally treating metals to decrease corrosion is still insufficient. Choudhuri *et al.* [9] offered a novel method, cold spraying bio-ceramic coatings onto metals at temperatures below their melting points (metal melting point). The composite powders used in this research are composed of titanium and HAP, with a proportion of HAP as high as 30 %. The research also found that the ratio of HAP deposition to HAP in the coating solution decreased with time. The binding strength for the deposit was also similar to that of plasma-sprayed HAP. The electrophoretic deposition (EPD) often used in thin-film fabrication was used to apply HAP coatings on SS316L surfaces in an investigation by Fadli *et al.* [10]. Three different voltage impacts of 40, 50, and 60 V on the characteristics of the coating layer were investigated. Quantitative analysis of Ca and P in HAP coatings was also conducted. During the corrosion testing, the release of Ni-ion from uncoated and coated materials was confirmed. In addition, the Vickers microhardness and wear test were used to assess the coating's mechanical properties, and the results of these tests are shown below. The development of the HAP layer was confirmed by the XRD of the coated sample. An increase in the number of pulses significantly enhanced the microstructure and growth of the HAP film, as shown by SEM. However, Jafari *et al.* [11] used the electrophoretic deposition approach to coat synthetic HAP on 316L for varying amounts of time (between 1 and 5 minutes) while maintaining a constant potential of 60 V. Electrochemical studies were conducted on bare and HAP-coated SS316L in biomimetic conditions. HAP-coated samples display a more noble change in the corrosion potential and corrosion current density compared to uncoated samples regarding the corrosion properties derived using open circuit potential and potential dynamic polarization. Rakngarm *et al.* [12] created a bio-active coating by employing a layer of HAP on metal-made implants within the humanoid body to take advantage of the mechano-chemical characteristic of metal-made implants and the bio-medical compatibility of human body tissues for the HAP surface.

A literature survey indicates that compared to uncoated SS316L, the corrosion resistance of SS316L treated with a HAP layer is much higher [13]. Therefore, there is a need to study the mechano-chemical properties of the HAP powder-coated SS 316L to protect it against corrosion and biodegradation. In this context, a literature review is carried out to assess the mechano-chemical characteristics of SS316L, HAP, and HAP-coated SS316L.

**Biomedical materials**

*Substrates*

Among the many materials used in medicine, the stainless-steel type (SS 316L) is a popular choice for implants in orthopedic surgery because of its resistance to corrosion, strong mechanical capabilities, and low cost. Hip and knee replacement pins, screws, and other orthopedic implants are often made of stainless steel. However, scientific trials reveal that the corrosion from SS316L implants results in the release of metal ions from implants into the body tissues, which might have adverse effects. Also, the fact that corrosion failures have occurred while using devices made from these materials within the human body has paved the way for many studies to make these materials more biocompatible and corrosion-resistant. Mechanical properties of SS 316L and bone were tested on the tensile testing machine. Figures 1 and 2 illustrate the stress-strain diagram of SS316L and bone material, respectively. Table 1 compares the mechanical properties of SS316L to the natural bone. In this work, the elemental composition of SS 316L was assessed by Oxford Instruments-manufactured Foundry Master Spectrometer (Uedem, Germany). Table 2 shows an elemental analysis range for SS316L. The chemical composition for SS316L shows good agreement with the literature data [14-18].

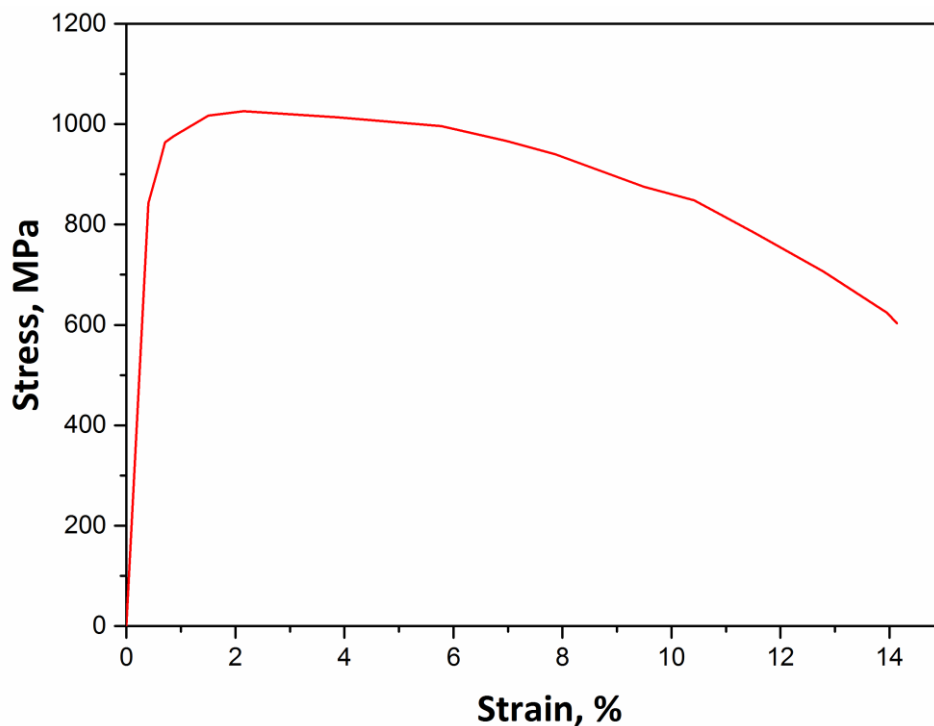

**Figure 1.** Stress-strain diagram of SS 316L

**Table 1.** Various mechanical properties of bone and SS 316L

No.	Properties	316L	BONE
1	Elastic modulus, GPa	210	10-30
2	Tensile stress, MPa	485	70-15
3	Tensile yield stress, MPa	170	120

**Table 2.** Elemental composition for SS 316L

Element	C	Mn	Si	Co	P	S	Cr	Mo	Ni	Fe
Content, wt.%	0.005	1.02	0.135	1.69	0.083	0.005	16.60	1.69	10.35	Balance

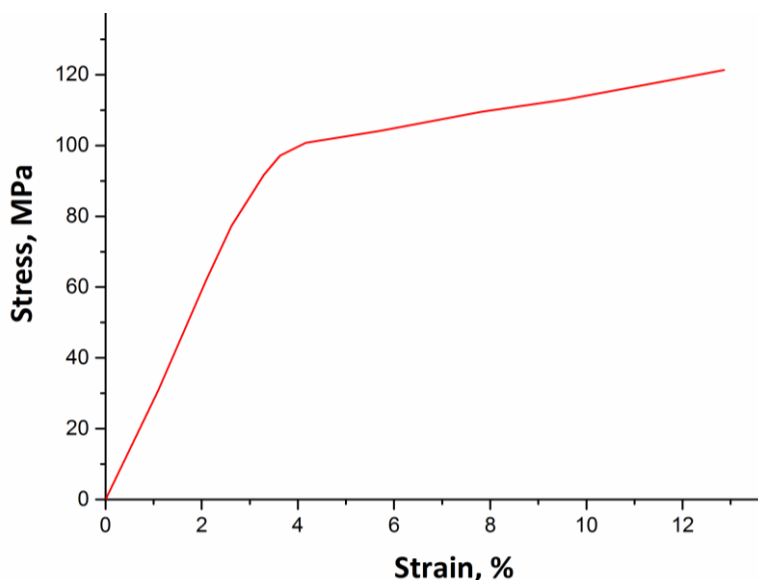


Figure 2. Stress-strain diagram of bone material

Hydroxyapatite: structure and properties

A ceramic material known for its medical applications is hydroxyapatite [19]. The bone material is composed of apatites which act as packing for Ca, Mg, P, and Na to strengthen the skeleton. Mineral HAP apatites ( $\text{Ca}_{10}(\text{PO}_4)_6(\text{OH})_2$ ) and brushite ( $\text{CaHPO}_4 \times 2\text{H}_2\text{O}$ ) have structural similarities with biological apatites. There are two stable calcium phosphate phases in bodily fluid and temperature: the brushite phase at ( $\text{pH} < 4.2$ ) and the HAP phase at ( $\text{pH} > 4.2$ ). Crystals of hydroxyapatite have a hexagonal, rhombic prism shape. Hydroxyapatite has the lattice configuration ( $a = 0.9432 \text{ nm}$ ) and ( $c = 0.6881 \text{ nm}$ ), as given in Figure 3. Corners of the base plane are hotspots for producing hydroxyl ions ( $\text{OH}^-$ ). Ions are arranged to be parallel to the c-axis of the crystals and transverse to the base plane of the crystals at every  $0.344 \text{ nm}$  ( $1/2$  of the unit cell).


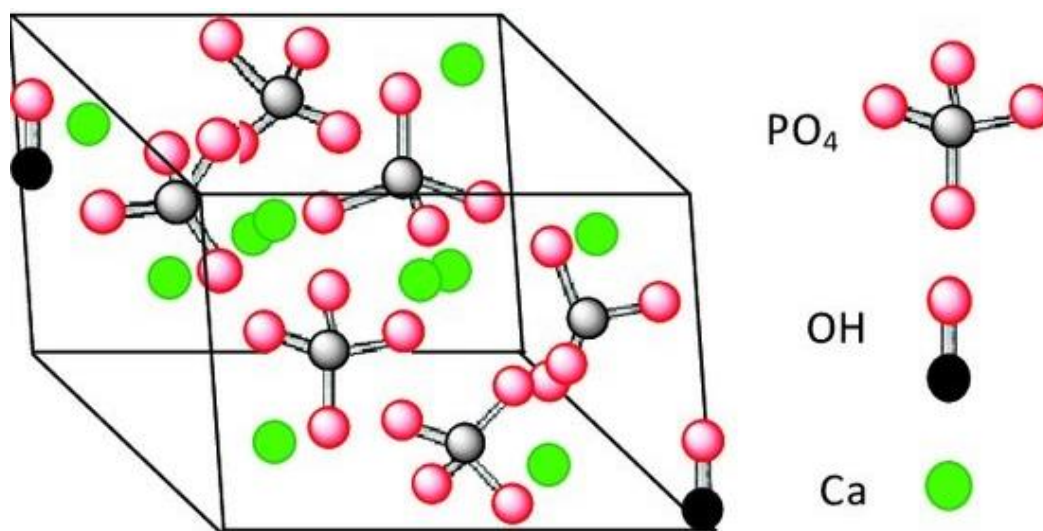


Figure 3. Simplified crystal structure of hydroxyapatite [21].  
(CC BY 4.0 Attribution)

Thus, about sixty percent of the Ca-ions in the crystal lattice are linked to the OH ions. HAP has a density of  $3.219 \text{ g cm}^{-3}$  [20]. HAP utilized in bones, hip replacement, and dental metal implants are generating around \$2.3 billion in yearly sales, which is expected to rise. The success of implants is contingent on many aspects, including those related to biocompatibility and mechanical features.

Owing to corrosion concerns, the use of metals within the human body has been minimal. Morphologically, the HAP powder seems blocky and irregular in shape, as presented in Figure 4.

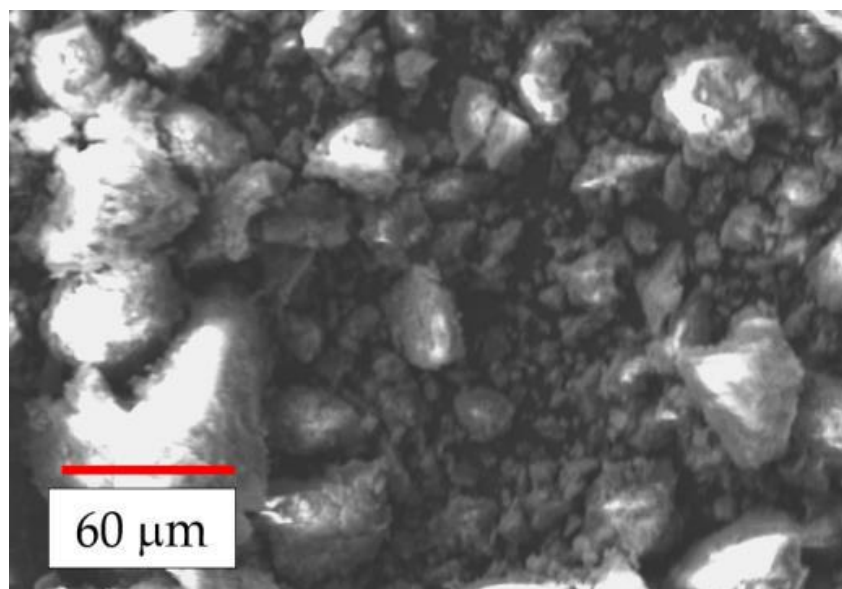

**Figure 4.** SEM image of hydroxyapatite powder [22]  
(CC BY 4.0 Attribution)

### Coatings

Surface engineering plays a crucial role in protecting biomaterials used in implants. It protects against corrosion, biodegradation, and erosion [18,23-38]. Various coating processes are used to enhance the surface of engineering and biomedical materials [39-42]. Electroplating, electroless plating, hot dipping [43-49], vapor deposition techniques (physical [50-56], chemical [57-59] and electrochemical [60]), thermal spraying [61-63], claddings [64-75], plasma spraying [76-83], and electrophoretic deposition are all methods used to deposit coatings onto metals (EPD). As seen in Figure 4, the size of HAP powder depicts that larger as well as smaller particles were present. Moreover, the particle melting and layer formation phenomenon depends upon the coating technology as well as particle properties. Therefore, the HAP can be deposited to different materials in different thicknesses by following the different procedures, as illustrated in Figure 5. Figure 6(a) presents the SEM images of HAP coating on Ti6Al4V. Figure 6(b) presents the XRD of the HAP electrodeposited coating, which shows the presence of different crystals, namely stoichiometric HAP and -tricalcium phosphate (-TCP) in the as-coated surface.

### Natural bone

In its mature form, bone is a biphasic composite. Collagen, a kind of protein, and HAP, a mineral phase that does not undergo chemical reactions, are its primary components. It is difficult to determine which phase is the primary load-bearer; maybe crystal serves as a filler to harden the collagen by limiting its mobility when stressed. Collagen is just 1 % as rigid as the mineral. Thus, it can't be relied upon to support bending or compressive forces. Only collagen contributes to the bone's fibrous structure. HAP is twice as powerful and significantly more rigid (Table 3).

Bone development involves inserting tiny platelets of HAP into predetermined pores in collagen, creating a composite of around two-thirds inorganic. Because of this, the fiber comparison only

works if it is considered a composite itself, reinforced with platelets because the bone is not homogenous even at the morphological level [85].

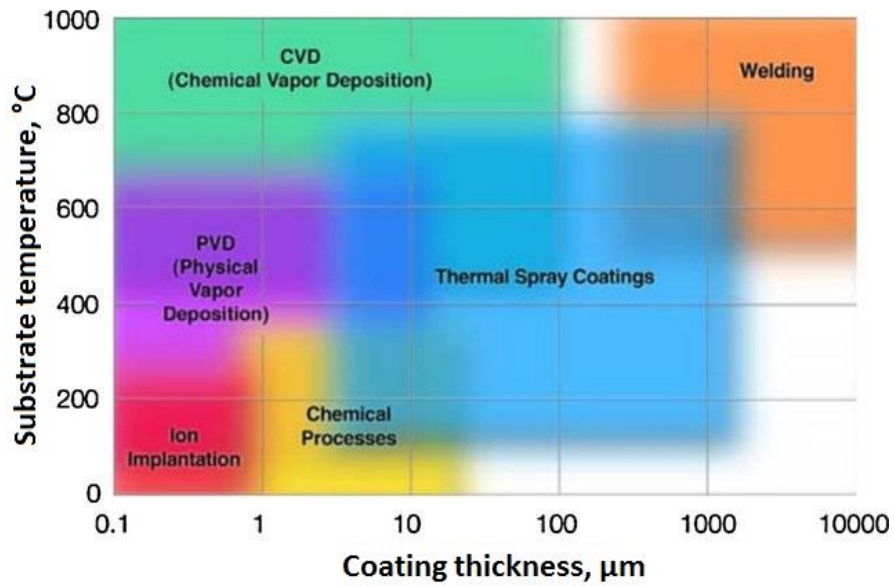


Figure 5. Substrate temperature versus thickness of coatings deposited by different processes [84] (CC BY 4.0 Attribution)


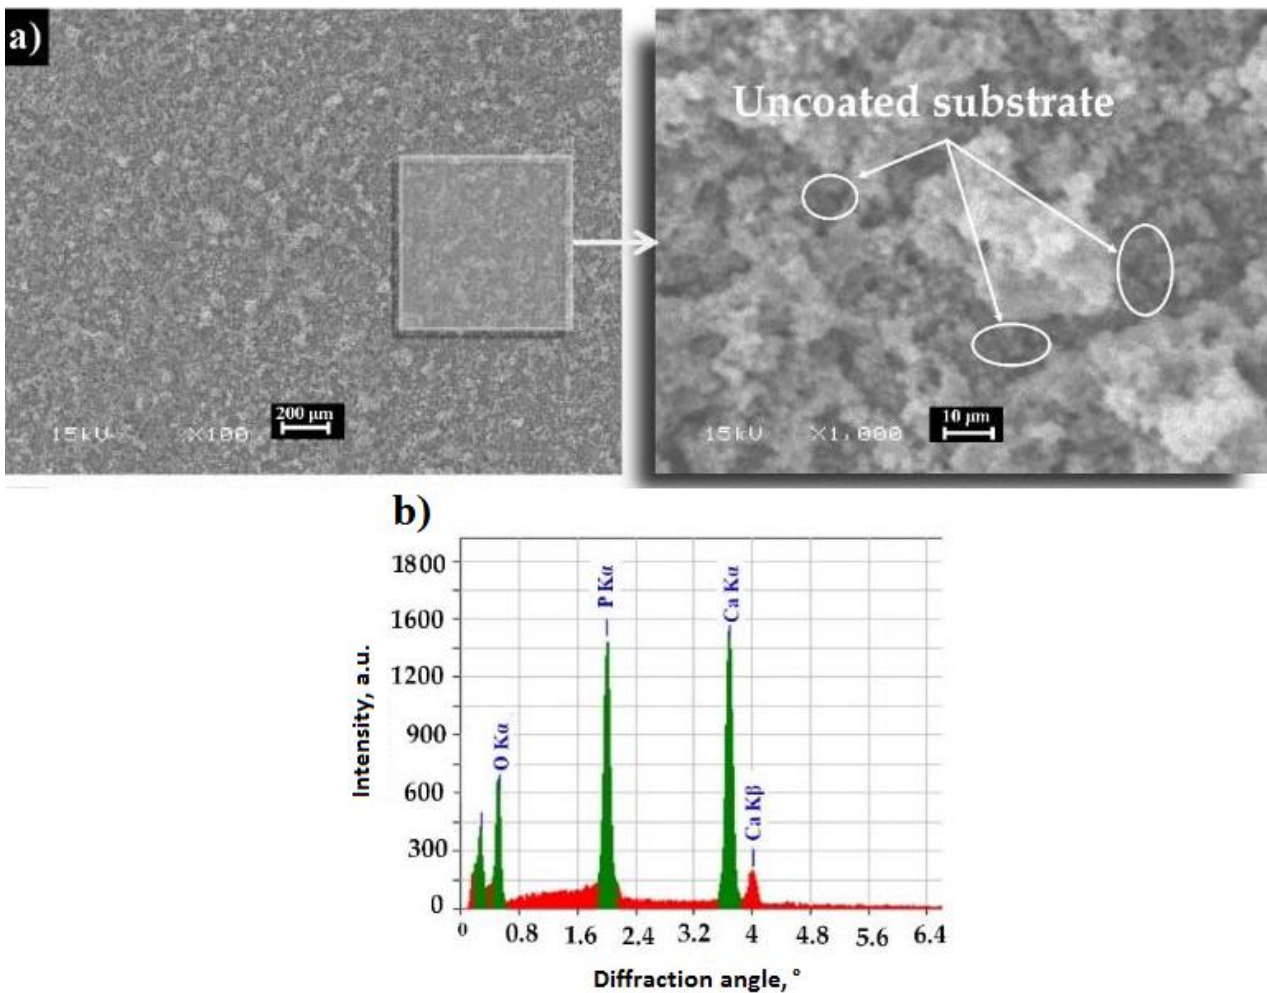


Figure 6. (a) SEM and (b) XRD of hydroxyapatite [22] (CC BY 4.0 Attribution)

**Table 3.** Material properties of the bone material [86]

No.	Feature	Value
1	HAP ultimate strain	0.001
2	HAP strength, GPa	0.1
3	Collagen's strength, MPa	50
4	HAP stiffness, GPa	130
5	Stress acting on collagen for 0.001 strain, MPa	1


Figure 7 illustrates that bone has a complicated hierarchical structure that has an effect on its mechanical performance. The magnitude and direction of the stresses that bones can withstand and how these stresses are transmitted to the rest of the body are both controlled by the density and configuration of mineralized platelets. There are two primary ways in which collagen fibrils may be arranged: firstly, randomly (woven bone), and secondly, in layers with desired orientation (lamellar bone). Primary lamellar bone consists of stacked layers of lamellae in a single plane, whereas secondary lamellar bone, Haversian bone, and woven bone all form cylindrical stacks of lamellae (laminar bone). In compact bone, you may find each kind [85]. An osteon is a fundamental unit of the skeletal structure. A hollow tube, approximately 200 m in diameter and 1-2 cm in length, serves as a weight-bearing component and a blood artery. Osteon walls are constructed using a coiled pattern of fine fibers (*i.e.* helical) of collagen interrupted by neighboring platelets of hydroxyapatite. As a consequence, compressive loads may be successfully carried by a small column, preventing buckling. However, its primary purpose is not durability [85].

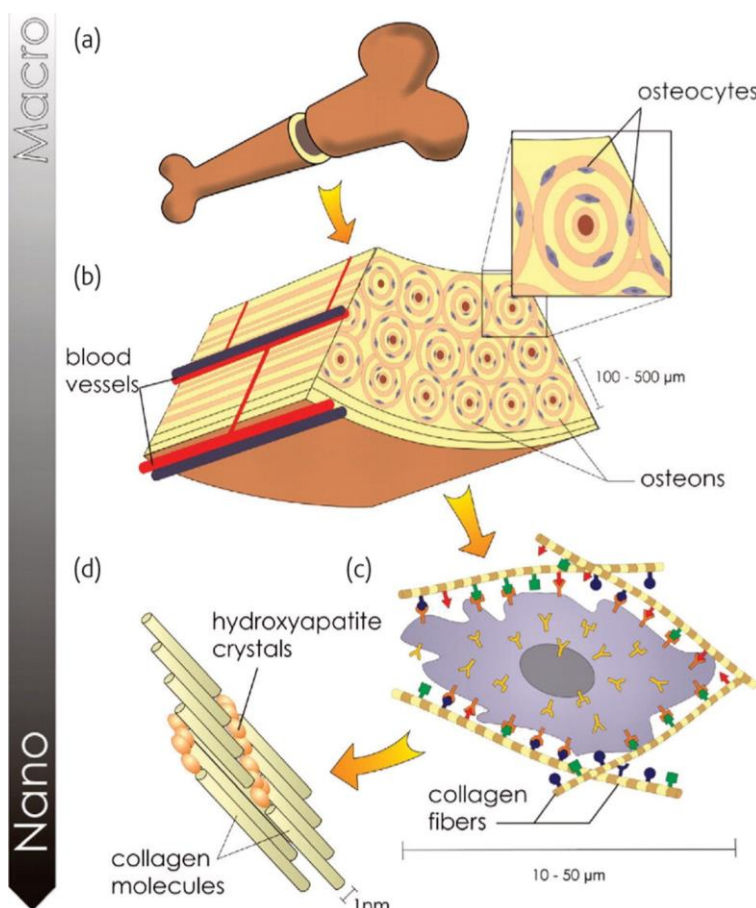

**Figure 7.** (a) Hierarchical structure of osseous tissue, (b) cylindrical Haversian systems or osteons, (c) cells are covered in a cluster of cell membrane receptors that react to particular binding sites, and (d) well-organized nano-structure of the surrounding extracellular matrix [91].  
(CC BY 4.0 Attribution)

## Conventional orthopedic

Sir John Charnley's groundbreaking research is essential to the current generation of implant designs [87]. The metallic component (named femoral) may be made of SS316L metallic alloys, such as cobalt-chromium-molybdenum, cobalt-nickel-chromium-molybdenum, or titanium-aluminum-vanadium alloys, while the UHMW (ultra-high molecular weight polyethylene) covering the femoral head may be manufactured of synthetic materials (Figure 8). PMMA bone cement is used to secure the devices in place. The current methods are temporary. As a result, 10 to 20 % of implants need replacement after 10 years, and some may require replacement even sooner, within the first 5 years [88]. Such short lifespans may be attributed to loosening, erosion-corrosion, the action of uneven loading, and irritation in the body tissues. Charnley [89] suggested that such types of implants can be used only for aged patients due to short life expectancy because of the very short lifetime for these implants owing to inadequate cement technology. A second characteristic that might interfere with implant function is stress shielding. Load misallocation at the bone-implant contact is a cause of implant dislocation or loosening [90]. This issue is present in all currently used metal implant components.

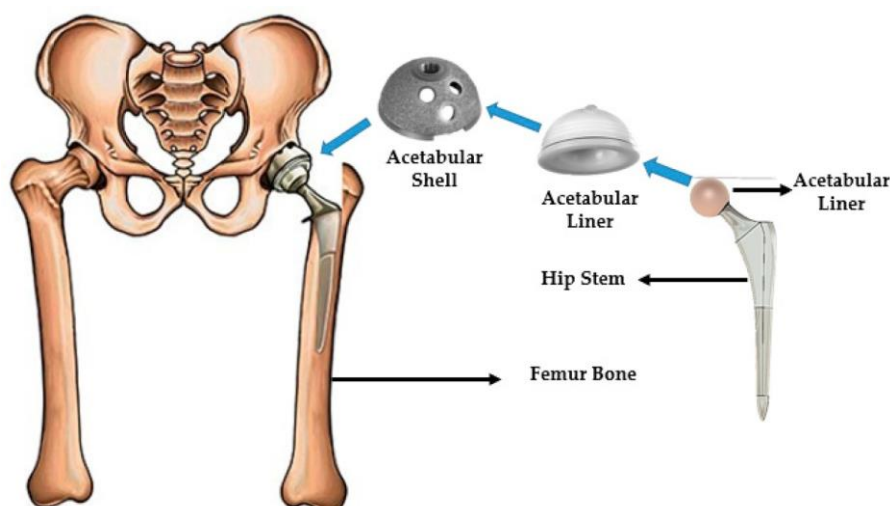

**Figure 8.** Model of an implanted total hip prosthesis [92]. (CC BY 4.0 Attribution)

## Conclusion and future prospective

In conclusion, metals may be used in a wide variety of contexts. And one of these sectors is medicine, which benefits from traits like strong strength, among many others. However, there is another side to metals: they tend to corrode when used in harsh environments like the one found within the human body. Although HAP has long been used to promote bone regeneration by conduction or as a scaffold for filling defects, recent advances in our understanding of its osteo-inductive characteristic indicate that it may soon play an even more important role in fostering new bone growth. Previously unimaginable clinical applications for HAP coatings are now a reality because of advances in technology. As a key component in the formation of calcified tissues, nanostructured calcium apatite is crucial. The nanostructured material may mimic the fundamental structure of bone and other calcification tissues by attaching biological molecules like proteins, and it can also synthesize controlled structures of apatite. Novel nanostructured biomimetic and biocompatible materials are needed for the regeneration process. Composites containing nanostructured bio-ceramic particles have the potential to increase the durability of injectable and controlled-setting synthetic bone implants and bone cements. The potential of nanotechnology for bone regeneration is the subject of

intensive study in the future. Additionally, nanostructured coatings have shown great promise in many other industrial applications. Therefore, HAP-based nanostructured coatings can be a topic of interest among researchers in the future. The coating is only one method that may protect these metals against corrosion or reduce their effects to an acceptable level. Additionally, as time went on, improvements were made to the coating process, and new coating materials were tested to find the healthiest and safest for human use. Several studies have shown that the combination of HAP with other metals increases the body's natural resistance to corrosion. Moreover, the HAP coating on Ti6Al4V has shown the uncoated surface sites with the electrodeposition process. Therefore, a suitable technique is required to be followed for future work.

## References

- [1] R. Langer, J. P. Vacanti, Tissue Engineering, *Science* **260** (1993) 920-926. <https://doi.org/10.1126/science.8493529>
- [2] S. Overgaard, H. M. Knudsen, L. N. Hansen, N. Mossing, Hip arthroplasty in Jutland, Denmark, *Acta Orthopaedica Scandinavica* **63** (1992) 536-538. <https://doi.org/10.3109/17453679209154731>
- [3] F. Cosman, S. J. de Beur, M. S. LeBoff, E. M. Lewiecki, B. Tanner, S. Randall, and R. Lindsay, Clinician's Guide to prevention and treatment of osteoporosis, *Osteoporos International* **25** (2014) 2359-2381. <https://doi.org/10.1007%2Fs00198-014-2794-2>
- [4] J. B. Park, *Biomaterials Science and Engineering*, Springer US, Boston, MA, 1984. <https://doi.org/10.1007/978-1-4613-2769-1>
- [5] M. López, G. Fuentes, R. González, J. González, E. Peón, C. Toledo, PMMA/Ca<sup>2+</sup> Bone cements: Part I. Physico chemical and thermoanalytical characterization, *Latin American Applied Research* **38** (2008) 227-234. <http://www.scielo.org.ar/pdf/laar/v38n3/v38n3a05.pdf>
- [6] M. Neville-Smith, L. Trujillo, R. Ammundson, Special Feature: Consistency in Postoperative Education Programs Following Total Hip Replacement, *Topics in Geriatric Rehabilitation* **15** (2000) 68-76. <https://doi.org/10.1097/00013614-200006000-00008>
- [7] D. Bhisare, P.K. Behera, *Synthesis and characterization of ultrafine hydroxyapatite (HAp) powder coating on stainless steel substrate by electrophoretic deposition*, National Institute of Technology, Rourkela, 2010. <https://core.ac.uk/download/pdf/53187495.pdf>
- [8] N. R. Babu, S. Manwatkar, K. P. Rao, T. S. Kumar, Bioactive coatings on 316L stainless steel implants, *Trends in Biomaterials and Artificial Organs* **17** (2004) 43-47. [https://e-tarjome.com/storage/btn\\_uploaded/2020-07-26/1595756035\\_10844-etarjome%20English.pdf](https://e-tarjome.com/storage/btn_uploaded/2020-07-26/1595756035_10844-etarjome%20English.pdf)
- [9] A. Choudhuri, P. S. Mohanty, J. Karthikeyan, *Bio-ceramic Composite Coatings by Cold Spray Technology*, in: *Proceeding of International Thermal Spray Conference by Japan Association of Earthquake Engineering*, Tokio, Japan, May 2009. [https://www.asbindustries.com/documents/paper\\_22241\\_manuscript\\_3762\\_final.pdf](https://www.asbindustries.com/documents/paper_22241_manuscript_3762_final.pdf)
- [10] A. Fadli, Komalasari, I. Indriyani, Coating Hydroxyapatite on 316L Stainless Steel Using Electroforesis Deposition Method, *Journal of Physics: Conference Series* **1351** (2019) 012015. <https://doi.org/10.1088/1742-6596/1351/1/012015>
- [11] S. Jafari, M. M. Atabaki, J. Idris, Comparative study on bioactive coating of Ti-6Al-4V alloy and 316 L stainless steel, *Metallurgical and Materials Engineering* **18** (2011) 145-158. [http://www.metalurgija.org.rs/mjom/vol18/No2/6\\_Jafari\\_MME\\_1802.pdf](http://www.metalurgija.org.rs/mjom/vol18/No2/6_Jafari_MME_1802.pdf)
- [12] A. Rakngarm, Y. Miyashita, Y. Mutoh, Formation of hydroxyapatite layer on bioactive Ti and Ti-6Al-4V by simple chemical technique, *Journal of Materials Science: Materials in Medicine* **19** (2008) 1953-1961 <https://doi.org/10.1007/s10856-007-3285-1>

- [13] N. Eliaz, T. M. Sridhar, U. K. Mudali, B. Raj, Electrochemical and electrophoretic deposition of hydroxyapatite for orthopaedic applications, *Surface Engineering* **21** (2005) 238-242 <https://doi.org/10.1179/174329405X50091>
- [14] W. Höland, Biocompatible and bioactive glass-ceramics — State of the art and new directions, *Journal of Non-Crystalline Solids* **219** (1997) 192-197. [https://doi.org/10.1016/S0022-3093\(97\)00329-3](https://doi.org/10.1016/S0022-3093(97)00329-3)
- [15] M. Long, H. Rack, Titanium alloys in total joint replacement — A materials science perspective, *Biomaterials* **19** (1998) 1621-1639. [https://doi.org/10.1016/S0142-9612\(97\)00146-4](https://doi.org/10.1016/S0142-9612(97)00146-4)
- [16] J. Singh, S. Kumar, S. K. Mohapatra, Erosion tribo-performance of HVOF deposited Stellite-6 and Colmonoy-88 micron layers on SS-316L, *Tribology International* **147** (2020) 105262. <https://doi.org/10.1016/j.triboint.2018.06.004>
- [17] J. Singh, S. Singh, Neural network supported study on erosive wear performance analysis of Y<sub>2</sub>O<sub>3</sub>/WC-10Co4Cr HVOF coating, *Journal of King Saud University - Engineering Sciences* (2022). <https://doi.org/10.1016/j.jksues.2021.12.005>
- [18] J. Singh, S. Singh, Neural network prediction of slurry erosion of heavy-duty pump impeller/casing materials 18Cr-8Ni, 16Cr-10Ni-2Mo, super duplex 24Cr-6Ni-3Mo-N, and grey cast iron, *Wear* **476** (2021) 203741. <https://doi.org/10.1016/j.wear.2021.203741>
- [19] R. J. Narayan, P. N. Kumta, C. Sfeir, D. H. Lee, D. Choi, D. Olton, Nanostructured ceramics in medical devices: Applications and prospects, *JOM* **56** (2004) 38-43. <https://doi.org/10.1007/s11837-004-0289-x>
- [20] J. B. Park, R. S. Lakes, *Biomaterials*, Springer US, Boston, MA, 1992. <https://doi.org/10.1007/978-1-4757-2156-0>
- [21] S. Rujitanapanich, P. Kumpapan, P. Wanjanoi, Synthesis of hydroxyapatite from oyster shell via precipitation, *Energy Procedia* **56** (2014) 112-117. <https://doi.org/10.1016/j.egypro.2014.07.138>
- [22] K. Khelifi, H. Dhiflaoui, A. Ben Rhouma, J. Faure, H. Benhayoune, A. Ben Cheikh Laarbi, Nanomechanical Behavior, Adhesion and corrosion resistance of hydroxyapatite coatings for orthopedic implant applications, *Coatings* **11** (2021) 477. <https://doi.org/10.3390/coatings11040477>
- [23] J. Singh, S. Kumar, S. K. Mohapatra, Optimization of erosion wear influencing parameters of HVOF sprayed pumping material for coal-water slurry, *Materials Today: Proceedings* **5** (2018) 23789-23795. <https://doi.org/10.1016/j.matpr.2018.10.170>
- [24] J. Singh, A review on mechanisms and testing of wear in slurry pumps, pipeline circuits and hydraulic turbines, *Journal of Tribology* **143** (2021) 090801. <https://doi.org/10.1115/1.4050977>
- [25] J. Singh, S. K. Mohapatra, S. Kumar, Performance analysis of pump materials employed in bottom ash slurry erosion conditions, *Jurnal Tribologi* **30** (2021) 73-89. <https://jurnaltribologi.mytribos.org/v30/JT-30-73-89.pdf>
- [26] J. Singh, S. Kumar, S. K. Mohapatra, Study on solid particle erosion of pump materials by fly ash slurry using Taguchi's orthogonal array, *Tribologia - Finnish Journal of Tribology* **38** (2021) 31-38. <https://doi.org/10.30678/fjt.97530>
- [27] J. Singh, H. S. Gill, H. Vasudev, Computational fluid dynamics analysis on effect of particulate properties on erosive degradation of pipe bends, *International Journal on Interactive Design and Manufacturing* (2022). <https://doi.org/10.1007/s12008-022-01094-7>
- [28] J. Singh, S. Singh, J. Pal Singh, Investigation on wall thickness reduction of hydropower pipeline underwent to erosion-corrosion process, *Engineering Failure Analysis* **127** (2021) 105504. <https://doi.org/10.1016/j.engfailanal.2021.105504>

- [29] J. Singh, *Application of thermal spray coatings for protection against erosion, abrasion, and corrosion in hydropower plants and offshore industry*, in *Thermal Spray Coatings*, L. Thakur, H. Vasudev (Eds.), 1st ed., CRC Press, Boca Raton, 2021, pp. 243-283. <https://doi.org/10.1201/9781003213185-10>
- [30] A. Biswas, L. Li, T. T. Maity, U. K. Chatterjee, B. B. Mordike, I. Manna, J. D. Majumdar, Laser surface treatment of Ti-6Al-4V for bio-implant application, *Lasers Engineering* **17** (2007) 59-73. <http://repository.ias.ac.in/18870/1/381.pdf>
- [31] J. Singh, S. Kumar, G. Singh, Taguchi's approach for optimization of tribo-resistance parameters for SS304, *Materials Today: Proceedings* **5** (2018) 5031-5038. <https://doi.org/10.1016/j.matpr.2017.12.081>
- [32] J. Singh, S. Kumar, S. K. Mohapatra, S. Kumar, Shape simulation of solid particles by digital interpretations of scanning electron micrographs using IPA technique, *Materials Today: Proceedings* **5** (2018) 17786-17791. <https://doi.org/10.1016/j.matpr.2018.06.103>
- [33] J. Singh, S. Kumar, S. Mohapatra, Study on role of particle shape in erosion wear of austenitic steel using image processing analysis technique, *Proceedings of the Institution of Mechanical Engineers, Part J: Journal of Engineering Tribology in Sustainable Advances in Manufacturing Processes* **233** (2019) 712-725. <https://doi.org/10.1177/1350650118794698>
- [34] J. Singh, S. Kumar, J. P. Singh, P. Kumar, S. K. Mohapatra, CFD modeling of erosion wear in pipe bend for the flow of bottom ash suspension, *Particulate Science and Technology* **37** (2019) 275-285. <https://doi.org/10.1080/02726351.2017.1364816>
- [35] J. Singh, J. P. Singh, M. Singh, M. Szala, Computational analysis of solid particle-erosion produced by bottom ash slurry in 90° elbow, *MATEC Web of Conferences* **252** (2019) 04008. <https://doi.org/10.1051/mateconf/201925204008>
- [36] J. Singh, *Investigation on slurry erosion of different pumping materials and coatings*, Thapar Institute of Engineering and Technology, Patiala, India, 2019. <https://tudr.thapar.edu:8443/jspui/handle/10266/5460>
- [37] S. Kumar, M. Singh, J. Singh, J. P. Singh, S. Kumar, Rheological characteristics of uni/bi-variant particulate iron ore slurry: Artificial neural network approach, *Journal of Mining Science* **55** (2019) 201-212. <https://doi.org/10.1134/S1062739119025468>
- [38] J. Singh, J. P. Singh, Numerical analysis on solid particle erosion in elbow of a slurry conveying circuit, *Journal of Pipeline Systems Engineering and Practice* **12** (2021) 04020070. [https://doi.org/10.1061/\(asce\)ps.1949-1204.0000518](https://doi.org/10.1061/(asce)ps.1949-1204.0000518)
- [39] H. Vasudev, P. Singh, L. Thakur, A. Bansal, Mechanical and microstructural characterization of microwave post processed Alloy-718 coating, *Materials Research Express* **6** (2020) 1265f5. <https://doi.org/10.1088/2053-1591/ab66fb>
- [40] H. Vasudev, G. Prashar, L. Thakur, A. Bansal, Microstructural characterization and electrochemical corrosion behaviour of HVOF sprayed Alloy718-nanoAl<sub>2</sub>O<sub>3</sub> composite coatings, *Surface Topography: Metrology and Properties* **9** (2021) 035003. <https://doi.org/10.1088/2051-672X/ac1044>
- [41] H. Vasudev, Wear characteristics of Ni-WC powder deposited by using a microwave route on mild steel, *International Journal of Surface Engineering and Interdisciplinary Materials Science* **8** (2020) 44-54. <https://doi.org/10.4018/IJSEIMS.2020010104>
- [42] H. Vasudev, G. Singh, A. Bansal, S. Vardhan, L. Thakur, Microwave heating and its applications in surface engineering, *Materials Research Express* **6** (2019) 102001. <https://doi.org/10.1088/2053-1591/ab3674>
- [43] Q. Wei, R. Haag, Universal polymer coatings and their representative biomedical applications, *Materials Horizons* **2** (2015) 567-577. <https://doi.org/10.1039/c5mh00089k>

- [44] J. Joseph, R. M. Patel, A. Wenham, J. R. Smith, Biomedical applications of polyurethane materials and coatings, *Transactions of the Institute of Metal Finishing* **96** (2018) 121-129. <https://doi.org/10.1080/00202967.2018.1450209>
- [45] R. N. Oosterbeek, C. K. Seal, J. M. Seitz, M. M. Hyland, Polymer-bioceramic composite coatings on magnesium for biomaterial applications, *Surface Coatings and Technology* **236** (2013) 420-428. <https://doi.org/10.1016/j.surfcoat.2013.10.029>
- [46] A. K. Hussain, U. M. B. Al Naib, Recent developments in graphene based metal matrix composite coatings for corrosion protection application: A review, *Journal of Metals, Materials and Minerals* **29** (2019) 1-9. <https://doi.org/10.14456/jmmm.2019.27>
- [47] J. Singh, S. Singh, R. Gill, Applications of biopolymer coatings in biomedical engineering, *Journal of Electrochemical Science and Engineering* (2022). <https://doi.org/10.5599/jese.1460>
- [48] J. Song, B. Winkeljann, O. Lieleg, Biopolymer-Based Coatings: Promising strategies to improve the biocompatibility and functionality of materials used in biomedical engineering, *Advanced Materials Interfaces* **7** (2020) 2000850. <https://doi.org/10.1002/admi.202000850>
- [49] Y. Guo, Y. Su, R. Gu, Z. Zhang, G. Li, J. Lian, L. Ren, Enhanced corrosion resistance and biocompatibility of biodegradable magnesium alloy modified by calcium phosphate/collagen coating, *Surface Coatings and Technology* **401** (2020) 126318. <https://doi.org/10.1016/j.surfcoat.2020.126318>
- [50] G. Singh, H. Vasudev, A. Bansal, S. Vardhan, S. Sharma, Microwave cladding of Inconel-625 on mild steel substrate for corrosion protection, *Materials Research Express* **7** (2020) 026512. <https://doi.org/10.1088/2053-1591/ab6fa3>
- [51] Y. Wang, J. Stella, G. Darut, T. Poirier, H. Liao, APS prepared NiCrBSi-YSZ composite coatings for protection against cavitation erosion, *Journal of Alloys and Compounds* **699** (2017) 1095-1103. <https://doi.org/10.1016/j.jallcom.2017.01.034>
- [52] F. Zhang, Y. Liu, Q. Wang, Y. Han, Z. Yan, H. Chen, Y. Tan, Fabricating a heavy oil viscosity reducer with weak interaction effect: Synthesis and viscosity reduction mechanism, *Colloid and Interface Science Communications* **42** (2021) 100426. <https://doi.org/10.1016/j.colcom.2021.100426>
- [53] S. S. Rajahram, T. J. Harvey, R. J. K. Wood, Erosion-corrosion resistance of engineering materials in various test conditions, *Wear* **267** (2009) 244-254. <https://doi.org/10.1016/j.wear.2009.01.052>
- [54] K. R. R. M. Reddy, N. Ramanaiah, M. M. M. Sarcar, Effect of heat treatment on corrosion behavior of duplex coatings, *Journal of King Saud University - Engineering Sciences* **29** (2017) 84-90. <https://doi.org/10.1016/j.jksues.2014.08.002>
- [55] A. F. Yetim, M. Y. Codur, M. Yazici, Using of artificial neural network for the prediction of tribological properties of plasma nitrided 316L stainless steel, *Materials Letters* **158** (2015) 170-173. <https://doi.org/10.1016/j.matlet.2015.06.015>
- [56] S. Buytoz, M. Ulutan, S. Islak, B. Kurt, O. N. Çelik, Microstructural and wear characteristics of high velocity oxygen fuel (HVOF) Sprayed NiCrBSi-SiC composite coating on SAE 1030 steel, *Arabian Journal for Science and Engineering* **38** (2013) 1481-1491. <https://doi.org/10.1007/s13369-013-0536-y>
- [57] J. Singh, S. Singh, A. Verma, Artificial intelligence in use of ZrO<sub>2</sub> material in biomedical science, *Journal of Electrochemical Science and Engineering* (2022). <https://doi.org/10.5599/jese.1498>
- [58] Y. Iwai, T. Miyajima, A. Mizuno, T. Honda, T. Itou, S. Hogmark, Micro-Slurry-jet Erosion (MSE) testing of CVD TiC/TiN and TiC coatings, *Wear* **267** (2009) 264-269. <https://doi.org/10.1016/j.wear.2009.02.014>

- [59] Z. Feng, Y. Tzeng, J. E. Field, Solid particle impact of CVD diamond films, *Thin Solid Films* **212** (1992) 35-42. [https://doi.org/10.1016/0040-6090\(92\)90497-Y](https://doi.org/10.1016/0040-6090(92)90497-Y)
- [60] U. B. Pal, S. C. Singhal, Electrochemical vapor deposition of Ytria-stabilized zirconia films, *Journal of Electrochemical Society* **137** (1990) 2937-2941. <https://doi.org/10.1149/1.2087102>
- [61] G. Prashar, H. Vasudev, Surface topology analysis of plasma sprayed Inconel625-Al<sub>2</sub>O<sub>3</sub> composite coating, *Materials Today: Proceedings* **50** (2022) 607-611. <https://doi.org/10.1016/j.matpr.2021.03.090>
- [62] G. Prashar, H. Vasudev, High temperature erosion behavior of plasma sprayed Al<sub>2</sub>O<sub>3</sub> coating on AISI-304 stainless steel, *World Journal of Engineering* **18** (2021) 760-766. <https://doi.org/10.1108/WJE-10-2020-0476>
- [63] G. Prashar, H. Vasudev, Structure-Property Correlation of Plasma-Sprayed Inconel 625-Al<sub>2</sub>O<sub>3</sub> Bimodal Composite Coatings for High-Temperature Oxidation Protection, *Journal of Thermal Spray Technology* **31** (2022) 2385-2408. <https://doi.org/10.1007/s11666-022-01466-1>
- [64] H. Vasudev, L. Thakur, H. Singh, A. Bansal, Erosion behaviour of HVOF sprayed Alloy718-nano Al<sub>2</sub>O<sub>3</sub> composite coatings on grey cast iron at elevated temperature conditions, *Surface Topography: Metrology and Properties* **9** (2021) 035022. <https://doi.org/10.1088/2051-672X/ac1c80>
- [65] P. Singh, H. Vasudev, A. Bansal, Effect of post-heat treatment on the microstructural, mechanical, and bioactivity behavior of the microwave-assisted alumina-reinforced hydroxyapatite cladding, *Proceedings of the Institution of Mechanical Engineers Part E Journal of Process Mechanical Engineering* (2022). <https://doi.org/10.1177/09544089221116168>
- [66] R. Singh, M. Toseef, J. Kumar, J. Singh, *Benefits and Challenges in Additive Manufacturing and Its Applications*, in: Sustainable Advances in Manufacturing and Materials Processing, S. Kaushal, I. Singh, S. Singh, A. Gupta (Eds.), 1st ed., CRC Press, Boca Raton, 2022, pp. 137-157. <https://doi.org/10.1201/9781003269298-8>
- [67] D. Kumar, R. Yadav, J. Singh, *Evolution and Adoption of Microwave Claddings in Modern Engineering Applications*, in: *Advances in Microwave Processing for Engineering Materials*, A. Bansal and H. Vasudev (Eds.), 1st ed., CRC Press, Boca Raton, 2022, pp. 134-153. <https://doi.org/10.1201/9781003248743-8>
- [68] H. Vasudev, G. Prashar, L. Thakur, A. Bansal, Electrochemical Corrosion Behavior and Microstructural Characterization of HVOF Sprayed Inconel-718 Coating on Gray Cast Iron, *Journal of Failure Analysis and Prevention* **21** (2021) 250-260. <https://doi.org/10.1007/s11668-020-01057-8>
- [69] H. Vasudev, L. Thakur, H. Singh, A. Bansal, A study on processing and hot corrosion behaviour of HVOF sprayed Inconel718-nano Al<sub>2</sub>O<sub>3</sub> coatings, *Materials Today: Proceedings* **25** (2020) 101626. <https://doi.org/10.1016/j.mtcomm.2020.101626>
- [70] G. Singh, A. Mehta, A. Bansal, Electrochemical behaviour and biocompatibility of claddings developed using microwave route, *Journal of Electrochemical Science and Engineering* **13(1)** (2023) 173-192 <https://doi.org/10.5599/jese.1604>
- [71] P. Singh, A. Bansal, H. Vasudev, P. Singh, In situ surface modification of stainless steel with hydroxyapatite using microwave heating, *Surface Topography: Metrology and Properties* **9** (2021) 035053. <https://doi.org/10.1088/2051-672X/ac28a9>
- [72] G. Prashar, H. Vasudev, L. Thakur, Influence of heat treatment on surface properties of HVOF deposited WC and Ni-based powder coatings: a review, *Surface Topography: Metrology and Properties* **9** (2021) 043002. <https://doi.org/10.1088/2051-672X/ac3a52>

- [73] G. Prashar, H. Vasudev, Structure-property correlation and high-temperature erosion performance of Inconel625-Al<sub>2</sub>O<sub>3</sub> plasma-sprayed bimodal composite coatings, *Surface Coatings and Technology* **439** (2022) 128450. <https://doi.org/10.1016/j.surfcoat.2022.128450>
- [74] G. Prashar, H. Vasudev, L. Thakur, Performance of different coating materials against slurry erosion failure in hydrodynamic turbines: A review, *Engineering Failure Analysis* **115** (2020) 104622. <https://doi.org/10.1016/j.engfailanal.2020.104622>
- [75] G. Singh, H. Vasudev, A. Bansal, S. Vardhan, Influence of heat treatment on the microstructure and corrosion properties of the Inconel-625 clad deposited by microwave heating, *Surface Topography: Metrology and Properties* **9** (2021) 025019. <https://doi.org/10.1088/2051-672X/abfc61>
- [76] J. Singh, Analysis on suitability of HVOF sprayed Ni-20Al, Ni-20Cr and Al-20Ti coatings in coal-ash slurry conditions using artificial neural network model, *Industrial Lubrication and Tribology* **71** (2019) 972-982. <https://doi.org/10.1108/ILT-12-2018-0460>
- [77] J. Singh, Wear performance analysis and characterization of HVOF deposited Ni-20Cr<sub>2</sub>O<sub>3</sub>, Ni-30Al<sub>2</sub>O<sub>3</sub>, and Al<sub>2</sub>O<sub>3</sub>-13TiO<sub>2</sub> coatings, *Applied Surface Science Advances* **6** (2021) 100161. <https://doi.org/10.1016/j.apsadv.2021.100161>
- [78] J. Singh, Tribo-performance analysis of HVOF sprayed 86WC-10Co4Cr & Ni-Cr<sub>2</sub>O<sub>3</sub> on AISI 316L steel using DOE-ANN methodology, *Industrial Lubrication and Tribology* **73** (2021) 727-735. <https://doi.org/10.1108/ILT-04-2020-0147>
- [79] J. Singh, J. P. Singh, Performance analysis of erosion resistant Mo<sub>2</sub>C reinforced WC-CoCr coating for pump impeller with Taguchi's method, *Industrial Lubrication and Tribology* **74** (2022) 431-441. <https://doi.org/10.1108/ILT-05-2020-0155>
- [80] K. Sunitha, H. Vasudev, Microstructural and Mechanical Characterization of HVOF-Sprayed Ni-Based Alloy Coating, *International Journal of Surface Engineering and Interdisciplinary Materials Science* **10** (2022) 5. <https://doi.org/10.4018/IJSEIMS.298705>
- [81] J. Singh, S. Kumar, S. K. Mohapatra, An erosion and corrosion study on thermally sprayed WC-Co-Cr powder synergized with Mo<sub>2</sub>C/Y<sub>2</sub>O<sub>3</sub>/ZrO<sub>2</sub> feedstock powders, *Wear* **438** (2019) 102751 <https://doi.org/10.1016/j.wear.2019.01.082>
- [82] J. Singh, S. Kumar, S. K. Mohapatra, Erosion wear performance of Ni-Cr-O and NiCrBSiFe-WC(Co) composite coatings deposited by HVOF technique, *Industrial Lubrication and Tribology* **71** (2019) 610-619. <https://doi.org/10.1108/ILT-04-2018-0149>
- [83] J. Singh, S. Kumar, S. K. Mohapatra, Tribological performance of Yttrium (III) and Zirconium (IV) ceramics reinforced WC-10Co4Cr cermet powder HVOF thermally sprayed on X2CrNiMo-17-12-2 steel, *Ceramics International* **45** (2019) 23126-23142. <https://doi.org/10.1016/j.ceramint.2019.08.007>
- [84] A. Billard, F. Maury, P. Aubry, F. Balbaud-Célérier, B. Bernard, F. Lomello, H. Maskrot, E. Meillot, A. Michau, F. Schuster, Emerging processes for metallurgical coatings and thin films, *Comptes Rendus Physique* **19** (2018) 755-768. <https://doi.org/10.1016/j.crhy.2018.10.005>
- [85] M. Elices, *Structural Biological Materials: Design and Structure-Property Relationships*, 1<sup>st</sup> ed., Elsevier & Pergamon Materials Series, 2000. ISBN: 978-0080434162.
- [86] J. F. V. Vincent, Strength and fracture of grasses, *Journal of Materials Science* **26** (1991) 1947-1950. <https://doi.org/10.1007/BF00543628>
- [87] R. C. Todd, C. D. R. Lightowler, J. Harris, Total Hip Replacement in Osteoarthritis using the Charnley Prosthesis, *British Medical Journal* **2** (1972) 752-755. <https://doi.org/10.1136/bmj.2.5816.752>

- [88] S. J. Birtwistle, K. Wilson, M. L. Porter, Long-term survival analysis of total hip replacement, *Annals of The Royal College of Surgeons of England* **78** (1996) 180-183. <http://www.ncbi.nlm.nih.gov/pmc/articles/pmc2502711/>
- [89] D. F. G. Emery, H. J. Clarke, M. L. Grover, Stanmore total hip replacement in younger patients: Review of a group of patients under 50 years of age at operation, *The Journal of Bone and Joint Surgery* **79** (1997) 240-246. <https://doi.org/10.1302/0301-620X.79B2.7165>
- [90] T. Karachalios, C. Tsatsaronis, G. Efraimis, P. Papadelis, G. Lyritis, G. Diakoumopoulos, The long-term clinical relevance of calcar atrophy caused by stress shielding in total hip arthroplasty, *The Journal of Arthroplasty* **19** (2004) 469-475. <https://doi.org/10.1016/j.arth.2003.12.081>
- [91] M. M. Stevens, J. H. George, Exploring and Engineering the Cell Surface Interface, *Science* **310** (2005) 1135. <https://doi.org/10.1126/science.1106587>
- [92] M. M. Soliman, M. E. H. Chowdhury, M. T. Islam, F. Musharavati, M. Nabil, M. Hafizh, A. Khandakar, S. Mahmud, E.Z. Nezhad, M.N.I. Shuzan, F.F. Abir, A review of biomaterials and associated performance metrics analysis in pre-clinical finite element model and in implementation stages for total hip implant system, *Polymers* **14** (2022) 4308. <https://doi.org/10.3390/polym14204308>

